


-15kV TOF: -9181 v  
 -3.6kV MCP: -3364 v  
 -2.4kV MCP: -1784 v  
 Input Cur: 312 ma  
 RPA max: 237 v  
 Mirror max: 238 v

Mon Oct 16 07:52:32 2006

## TIDE Direct Events

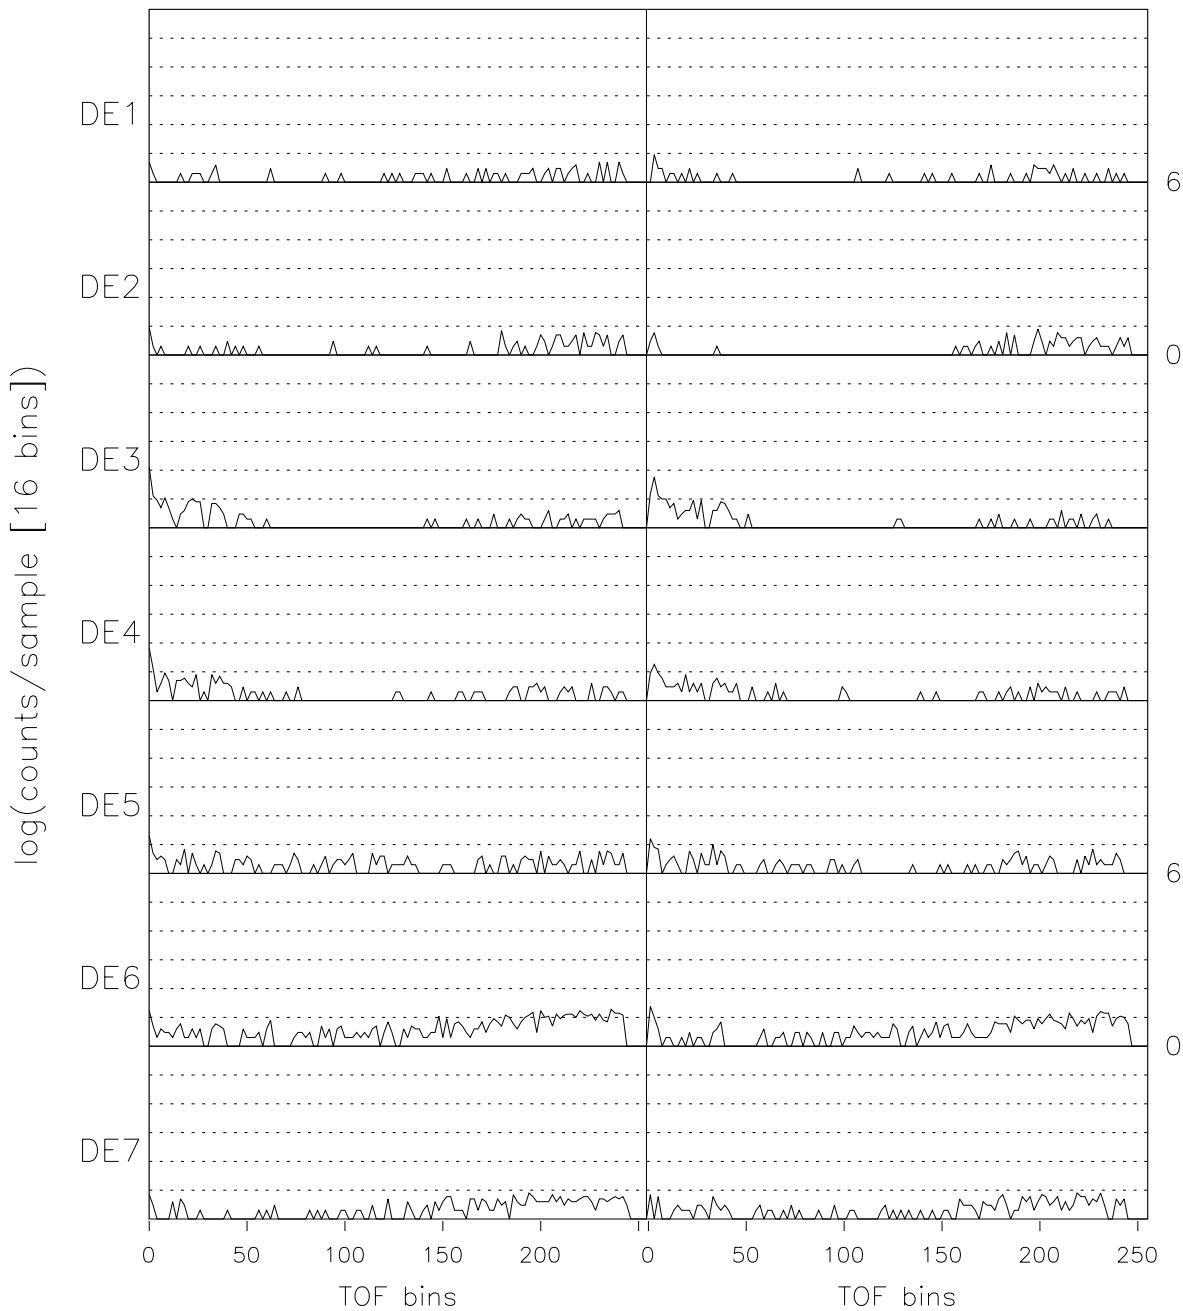

reported: 10-12-06 16:36:06 UT

reported: 10-12-06 16:39:18 UT

file: /export/data/tide/nrt/06101201.dat

-15kV TOF: -9181 v

-3.6kV MCP: -3364 v

-2.4kV MCP: -1784 v

Input Cur: 312 ma

RPA max: 238 v

Mirror max: 238 v